

FIG. 1



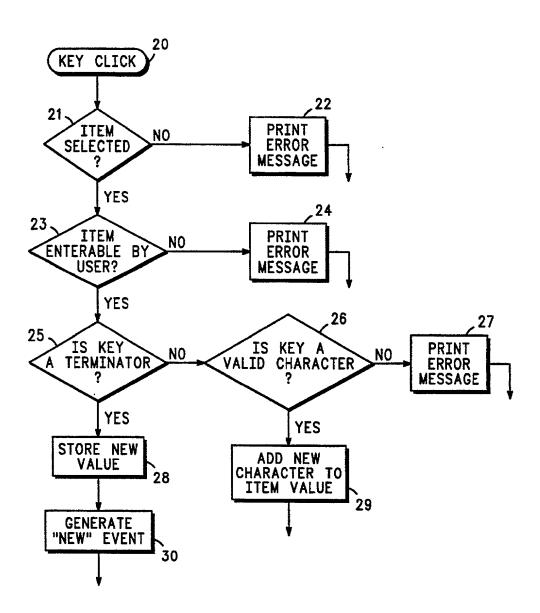


FIG. 2A



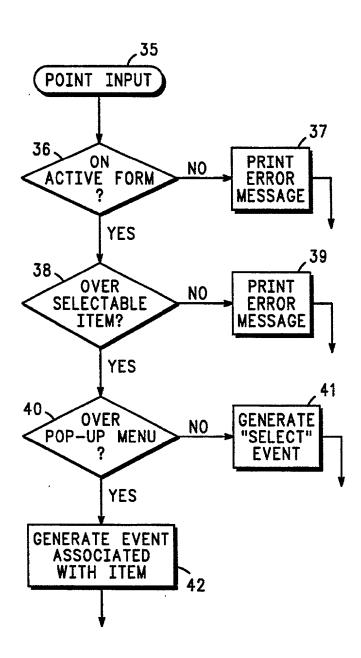


FIG. 2B

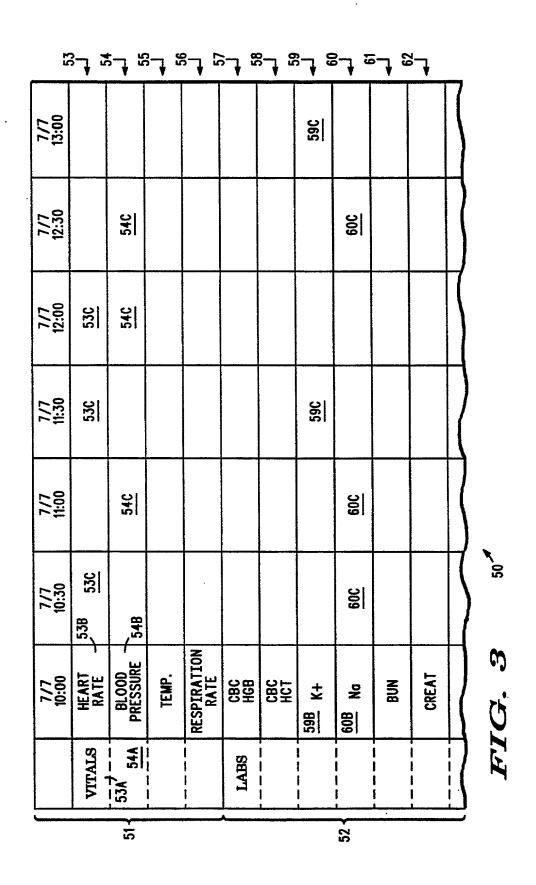


U.S. Patent

| 53'A | ,53 | ' ₍ 54 | , |
|--------------|------------------|-------------------|-------|
| | VITALS | <u>54'A</u> | |
| 7/7 10:00 | HEART , RATE | BLOOD PRESSURE | TEMP. |
| 7/7 10:30 | 53'B <u>53'C</u> | 54'B | |
| 7/7 11:00 | | 54'C | |
| 7/7 11:30 | <u>53'C</u> | | 7 |
| 7/7 12:00 | <u>53'C</u> | | |
| 7/7 12:30 | | <u>54'C</u> | |
| 7/7 13:00 | | | |
| 7/7 13:30 | | <u>54'C</u> | |
| 7/7 14:00 | | | |
| 7/7 14:30 | | | |
| 7/7 15:00 | | | |
| 7/7 15:30 | | <u>54'C</u> | |
| † FIG. 4 | | | |

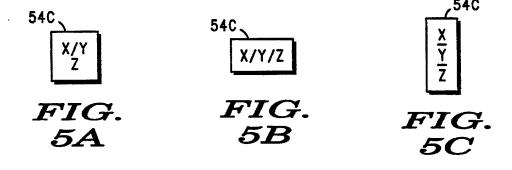

Sheet 6 of 10

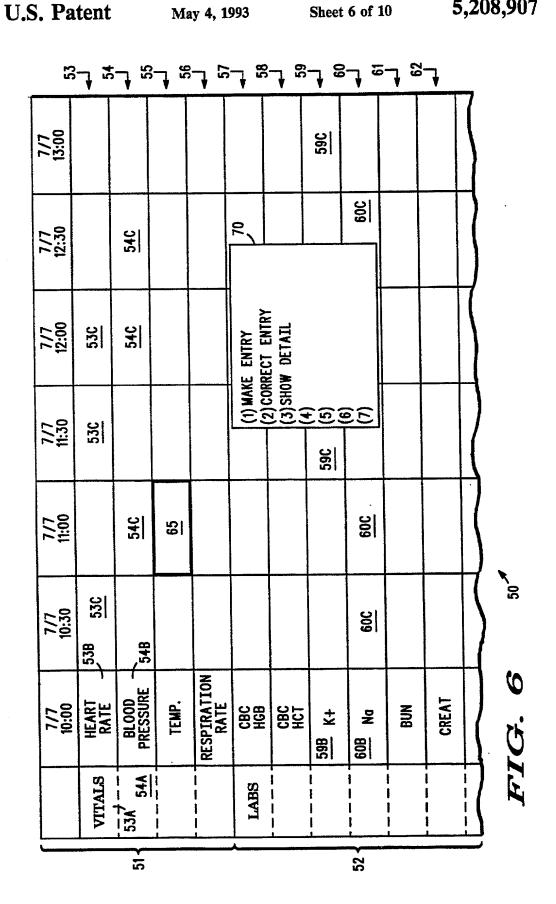

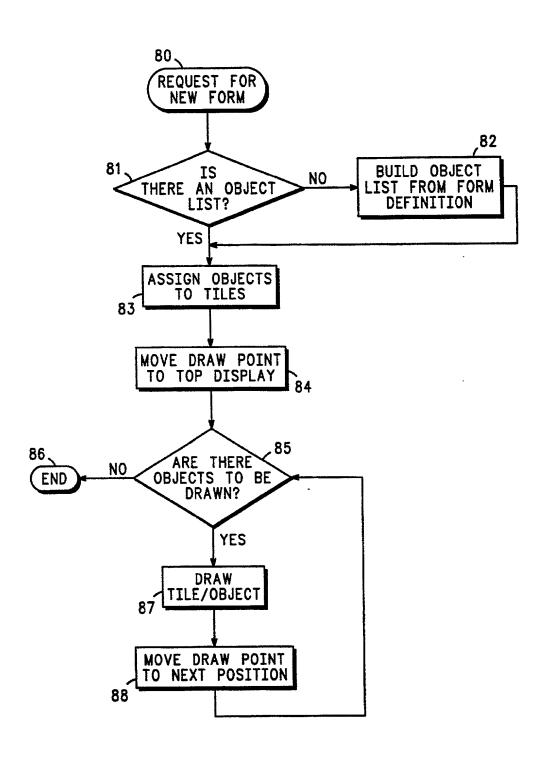
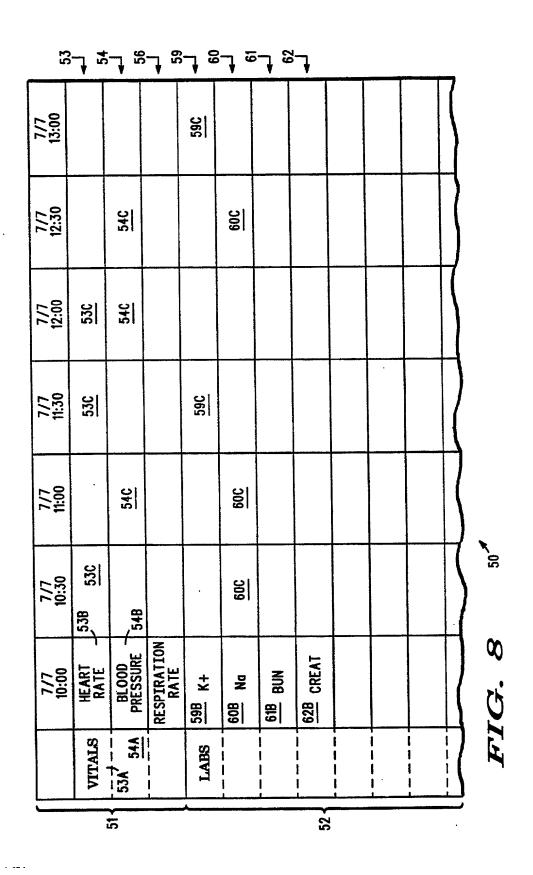
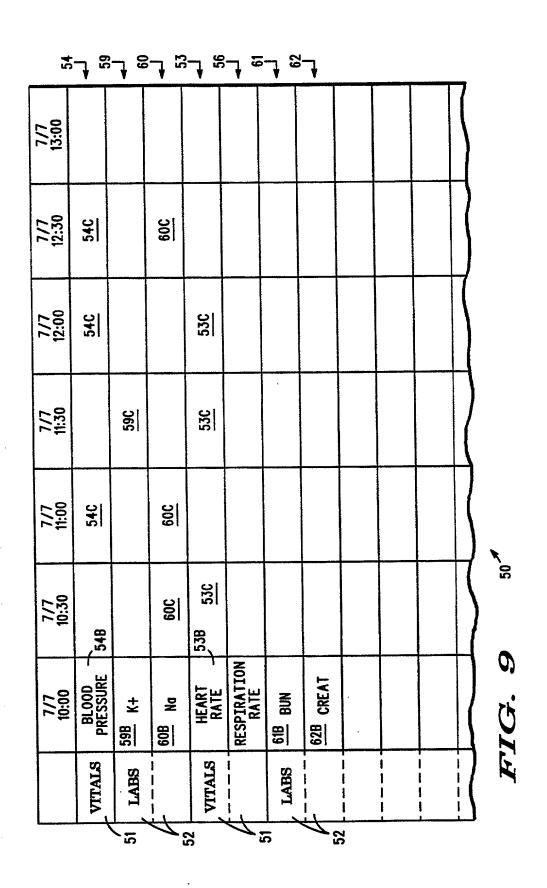


FIG. 7





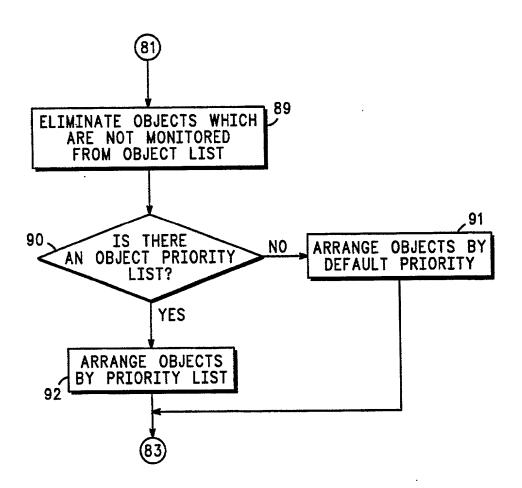


FIG. 10